



RC-17 Temperature Data Logger User Manual


1. If the data logger has not been stored at room temperature, place it in room temperature for 30 mins before starting.
2. Press and hold the START/STOP button for approximately 5 seconds. The green light flashes for 5 secs.
3. Place the data logger into the location to be monitored. Recording will begin after the start delay period shown on the logger.
4. If there has been no temperature excursion, the green light will flash green every 10 seconds. If a temperature excursion has occurred, the red light will flash every 10 seconds.
5. To stop recording, press and hold the START/STOP button for 5 seconds. The red light flashes for 5 secs.
6. To generate a trip report, tear or cut away the waterproof plastic bag. Be careful not to damage the device when cutting away the bag. Insert the logger into a PC USB port. The green and red lights will alternately flash when the PDF report is being generated.
7. When the PDF report has been generated, the green and red lights will illuminate solid until the logger is removed from the USB port.

OPERATION	ACTION	LED INDICATION
START Recording	Press the START/STOP Button for 5 seconds	The RECORD LED will blink 5 times
STOP Recording	Press the START/STOP Button for 5 seconds	The STATUS LED will blink 5 times

Status Indication

The status of the recording can be analyzed by the unit's indicator light.

STATUS	LED INDICATION
Does not Start	Red and green light flash simultaneously
Start-up Delay	Red and green light blinks alternately once
Start - Normal	Green light blinks once (flashes 10 times every minute)
Start - Alarm	Red light flashes once (flashes 10 times every minute)
Start - Mark	Red and green light flash 3 times at the same time
Start - Mark overrun	Red and green light flash 3 times alternately
Stop - Normal	Green light flashes twice
Stop - Alarm	Red light flashes twice

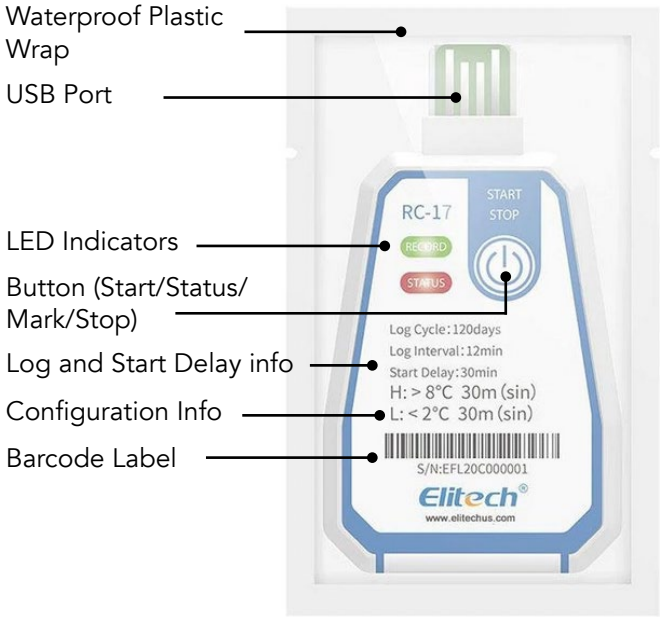

Front

- Waterproof Plastic Wrap
- USB Port
- LED Indicators
- Button (Start/Status/Mark/Stop)
- Log and Start Delay info
- Configuration Info
- Barcode Label



Back

- Start/Stop Info
- Mark Info
- Status Request
- Paste Area

Specifications

Temperature Measuring Range	-30°C ~ +70°C
Resolution	0.1°C
Accuracy	±0.5°C (@-20°C~+40); 1°C/(@others)
Memory Capacity	16000 readings
Recording Period	6, 15, 30, 60, 90, 120, 180 days (customisable)
Alarm Type	single or cumulative
Report Type	PDF format
Data Interface	USB2.0
Sensor type	Internal NTC
Power supply	Built-in CR2450 wide temperature lithium battery
Battery life	2 years (stored and used under normal temperature environment)
Protection grade	IP67
Dimension	93mm (L) x 58mm (W) x 8mm (H)
Weight	20g

Download Data





Press the STOP button for 5 secs to stop logging. The red light flashes 5 times. Take the logger out of the waterproof bag



Press the device into the computers USB port to view the PDF data report.

Report Content

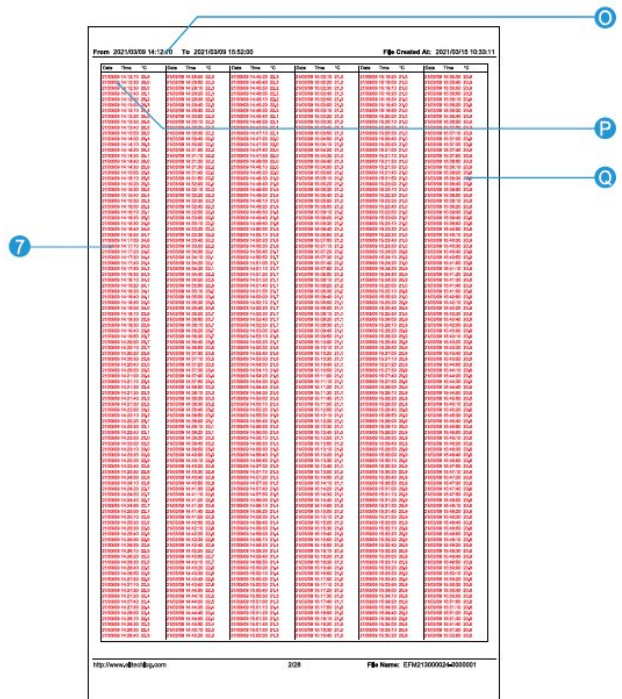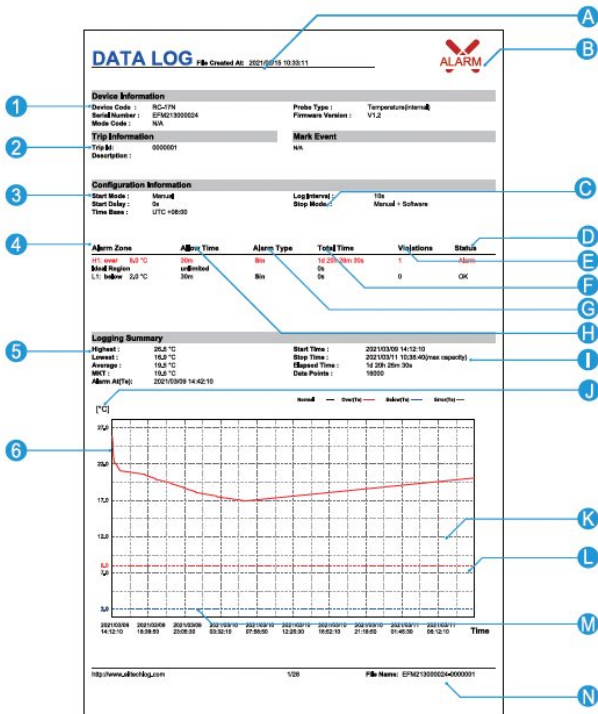

1 Basic product information	C Set stop method	K Alarm threshold line (corresponding to item L)
2 Descriptions (customizable)	D Alarm status of D alarm section	L Alarm threshold
3 Configuration information	E Total number exceeds the alarm threshold temperature	M Record data curve Note: ultra-high temperature is red, ultra-low temperature is blue, others are black
4 Alarm threshold and related statistics	F The total length of time that the F temperature exceeds the alarm threshold	N File name (serial number + purpose description ID)
5 Statistics	G Alarm delay and alarm type	O Recording time range in the current page
6 Temperature data graph	H Alarm threshold and alarm interval division	P Record when P date changes (date + temperature)
7 Temperature data details	I Stop time (actual stop method)	Q Record when Q date has not changed (time + temperature)
A File creation time (stop recording time)	J Data curve graph ordinate unit	